


Figure S3

A

	parameter	value
1	Cytokine	G-CSF
2	Vendor	Bio-Rad
3	Samples included in this agreement	32
4	Proportion of both readings in range	86.5
5	Limits of agreement	0.70 to 1.51
6	Constant variance p.value	0.003
7	Constant ratio p.value	0.249
8	Ratio is 1 p.value	0.454

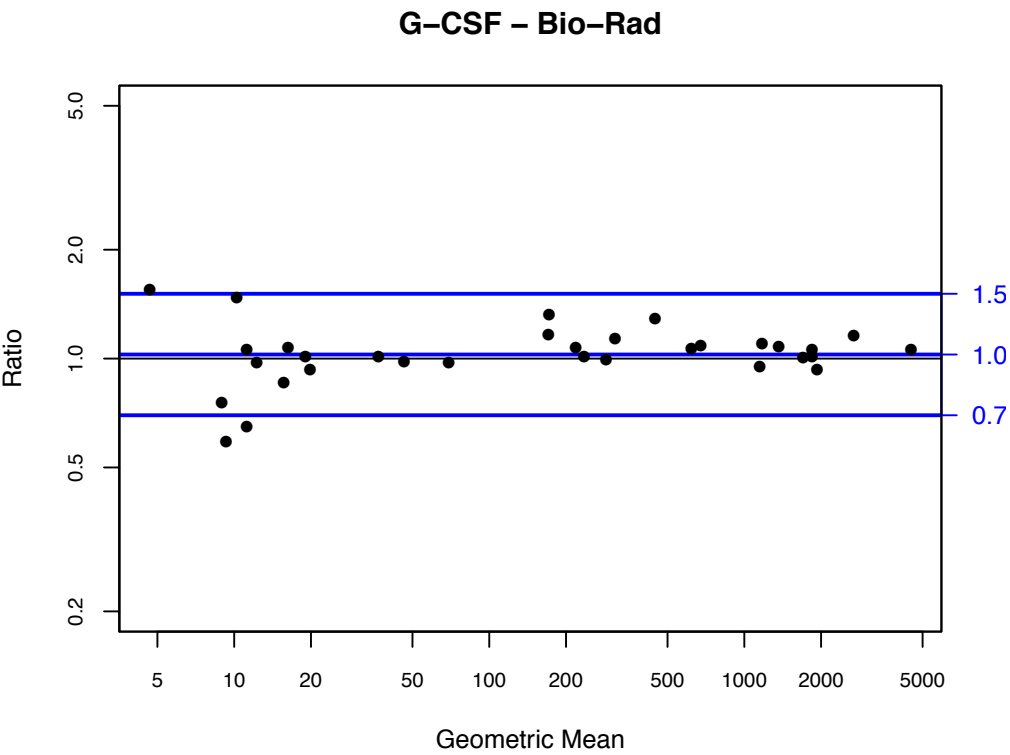

B

	parameter	value
1	Cytokine	G-CSF
2	Vendor	INV_MAG
3	Samples included in this agreement	26
4	Proportion of both readings in range	65.0
5	Limits of agreement	0.56 to 1.47
6	Constant variance p.value	0.096
7	Constant ratio p.value	0.143
8	Ratio is 1 p.value	0.059

