

CORRECTION

# Correction: Laboratory Evaluation of the Shinyei PPD42NS Low-Cost Particulate Matter Sensor

Elena Austin, Igor Novosselov, Edmund Seto, Michael G. Yost

The y-axis label for [Fig 5](#) incorrectly states mean rather than difference. The correct y-axis is “Difference of Shinyei and APS Mass ( $\mu\text{g}/\text{m}^3$ )”. The authors have provided a corrected version of [Fig 5](#) here.




 OPEN ACCESS

**Citation:** Austin E, Novosselov I, Seto E, Yost MG (2015) Correction: Laboratory Evaluation of the Shinyei PPD42NS Low-Cost Particulate Matter Sensor. PLoS ONE 10(10): e0141928. doi:10.1371/journal.pone.0141928

**Published:** October 28, 2015

**Copyright:** © 2015 Austin et al. This is an open access article distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

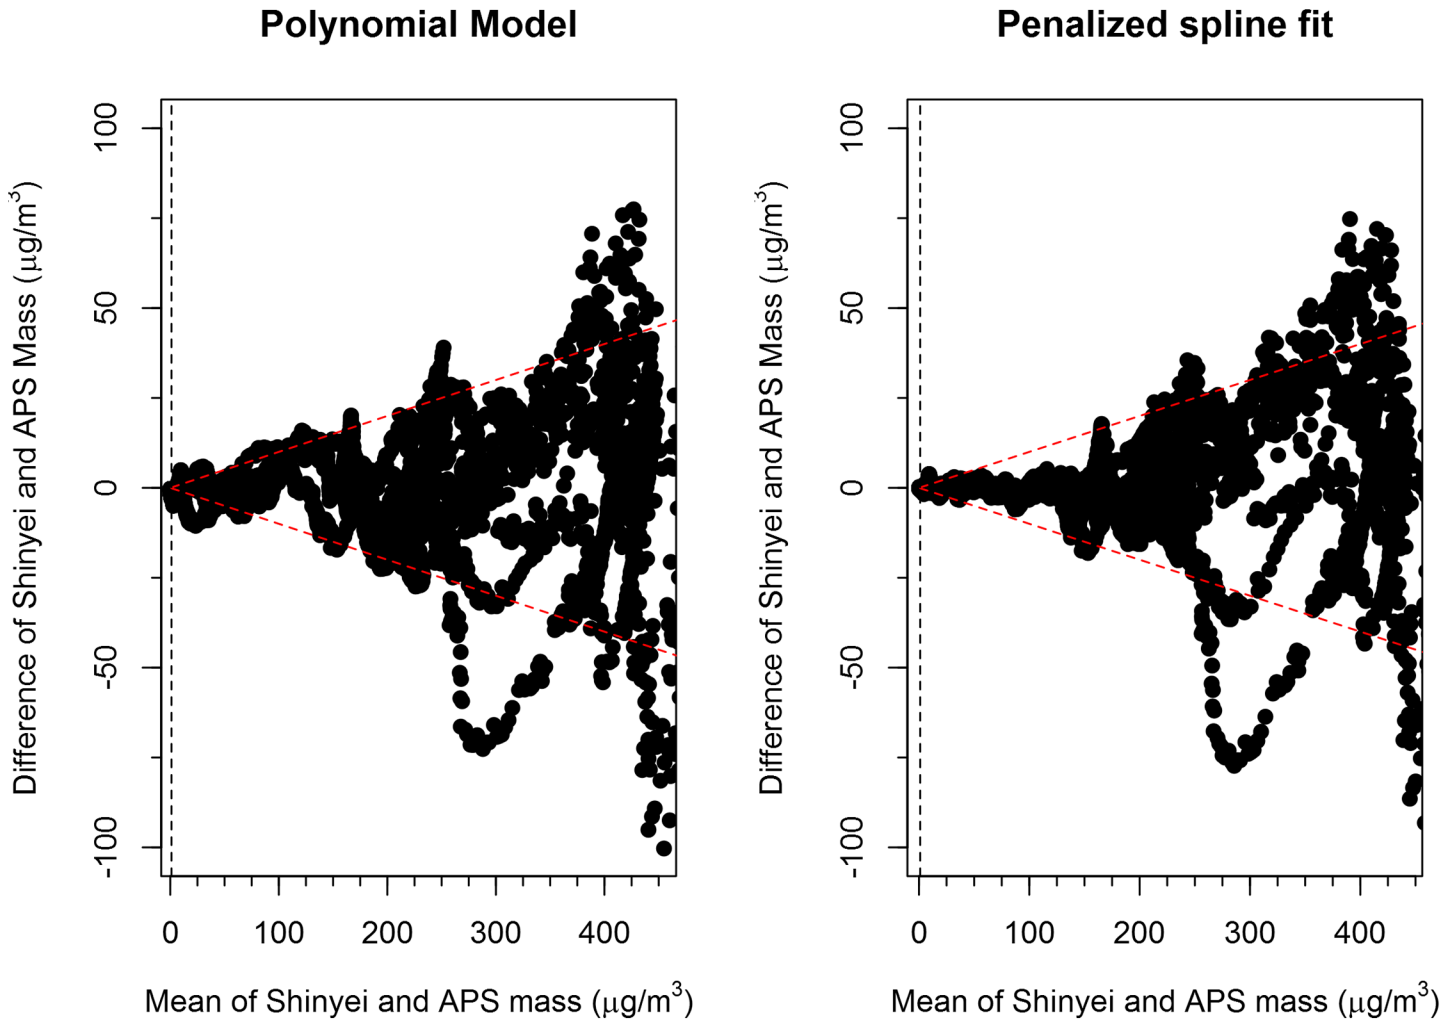

**Fig 5. Bland Altman Plots (4 sensors pooled together).** The red dashed lines represent a 10% error on the mass measurement. The black vertical dashed line represents the LOD.

doi:10.1371/journal.pone.0141928.g001

### Reference

1. Austin E, Novosselov I, Seto E, Yost MG (2015) Laboratory Evaluation of the Shinyei PPD42NS Low-Cost Particulate Matter Sensor. PLoS ONE 10(9): e0137789. doi:[10.1371/journal.pone.0137789](https://doi.org/10.1371/journal.pone.0137789) PMID: [26367264](https://pubmed.ncbi.nlm.nih.gov/26367264/)