



A. -ESI MRM(1239.8/79.0)

LpxH minus IPTG

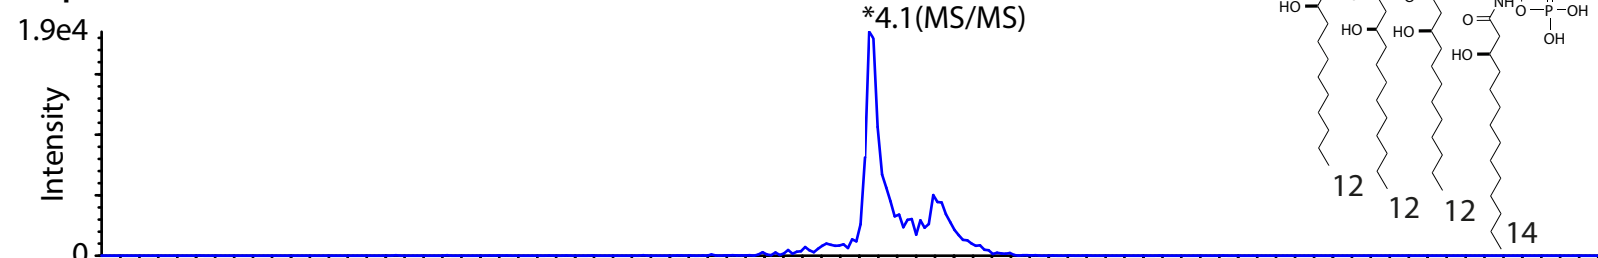


B. -ESI MRM(1267.8/79.0)

LpxH minus IPTG

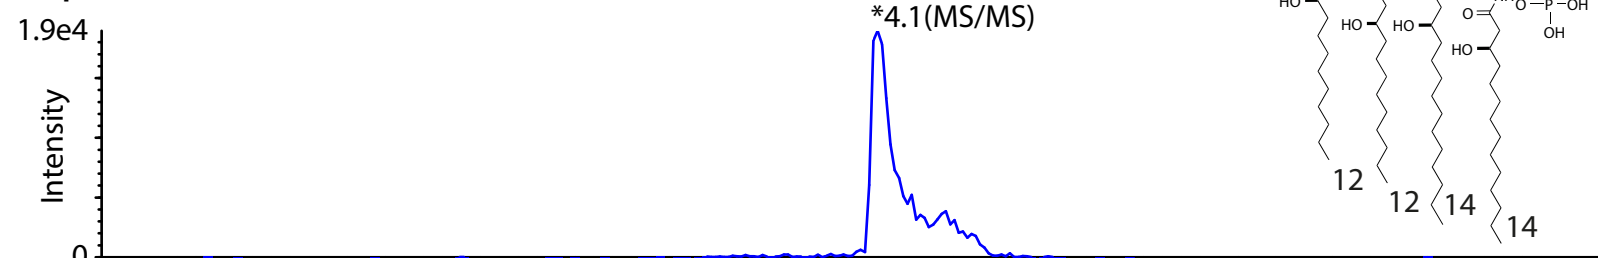


C. -ESI MRM(1323.9/79.0)

LpxH minus IPTG

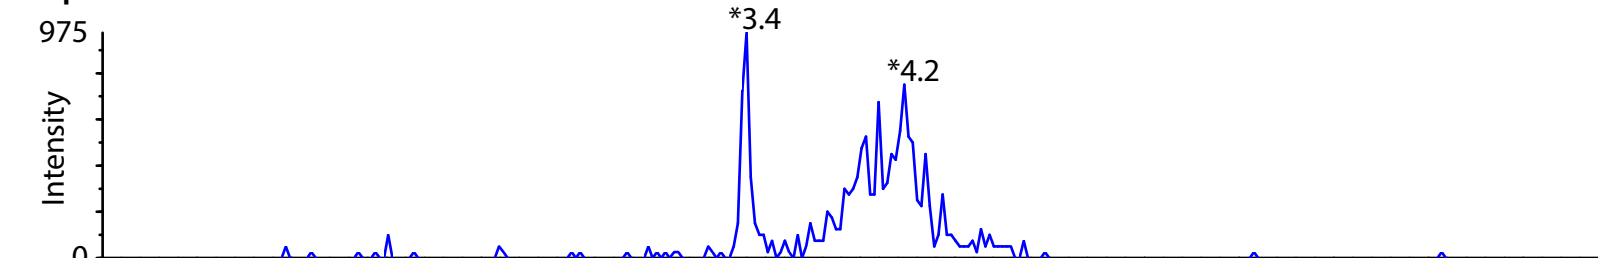


D. -ESI MRM(1239.8/79.0)

Standard DSMP

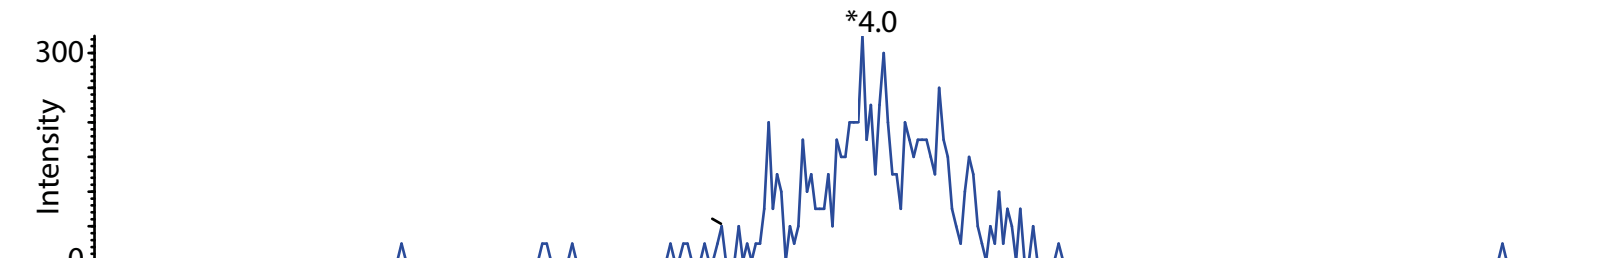


E. -ESI MRM(1267.8/79.0)

Standard DSMP

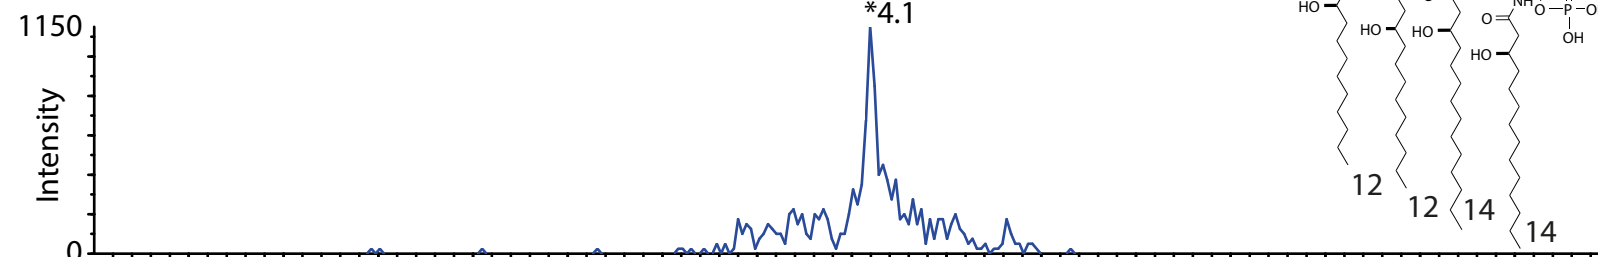


F. -ESI MRM(1323.9/79.0)

Standard DSMP

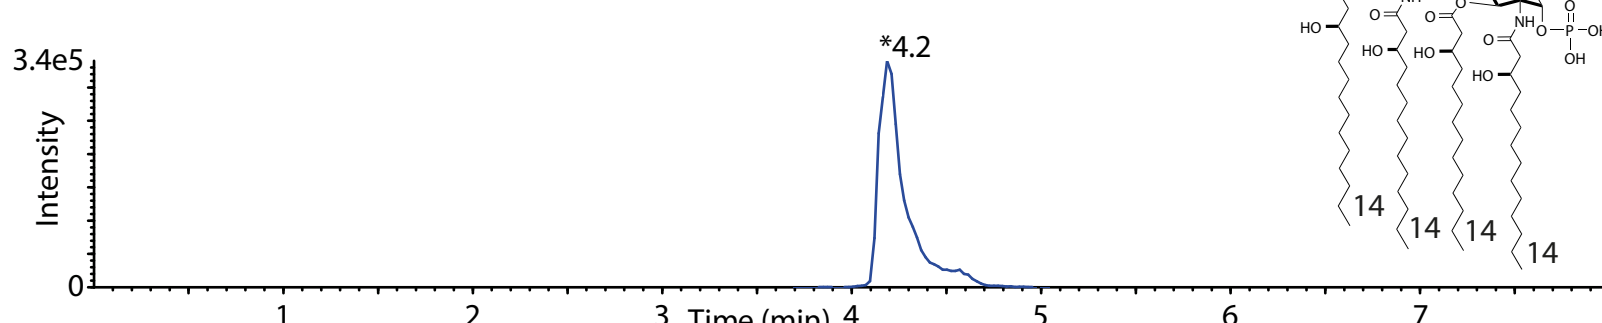


G. -ESI Product Ion Scan (1239.8) (rt 4.1-4.1 min, CE -75)

LpxH minus IPTG

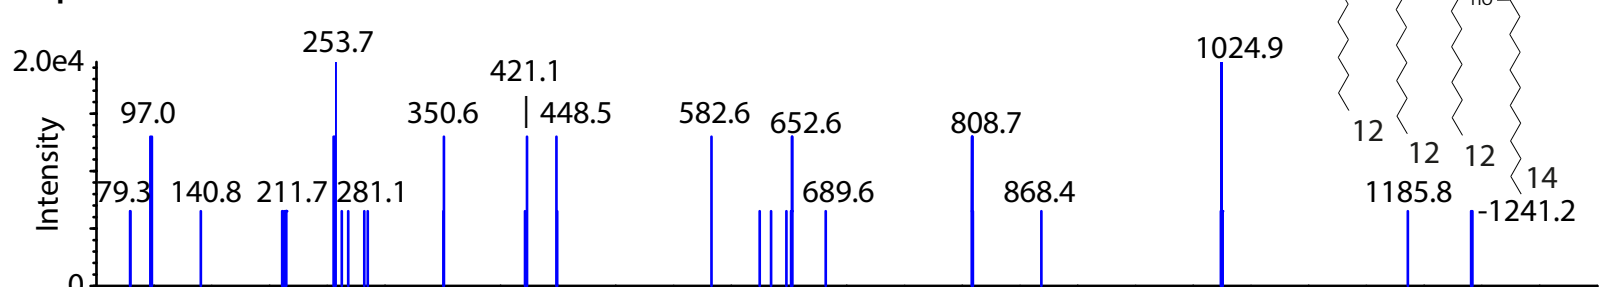

H. -ESI Product Ion Scan (1267.8) (rt 4.1-4.2 min, CE -75)

LpxH minus IPTG

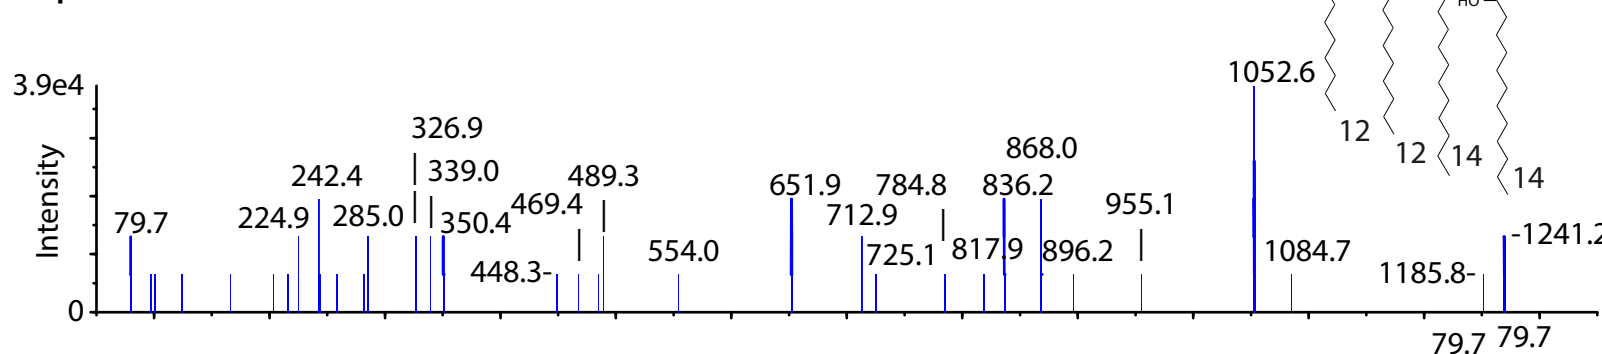

I. -ESI Product Ion Scan (1323.9) (rt 4.1-4.4 min, CE -75)

Standard DSMP

